

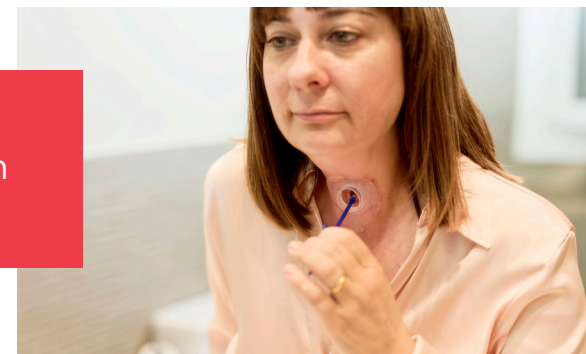


Provox ActiValve voice prosthesis (VP) is intended for those people who experience early central leakage (less than eight weeks). ActiValve has been found to have an average device life of 10 months.

Provox ActiValve works similarly to other Provox voice prostheses except it has magnets to help the valve stay closed. It does require additional maintenance and attention to precautions.

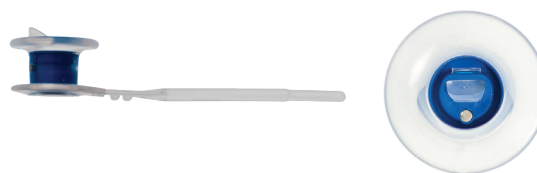


Maintaining your Provox ActiValve VP

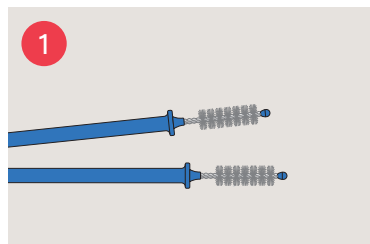


Provox ActiValve voice prosthesis comes with one Provox Brush for cleaning and a second Brush for lubricating.

► **LABEL** your cleaning Brush and your lubricating Brush so you know which is which.

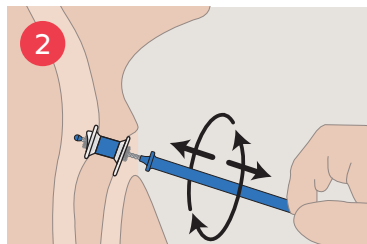


► **USE** the Brush labeled "Clean" to clean your voice prosthesis twice a day.

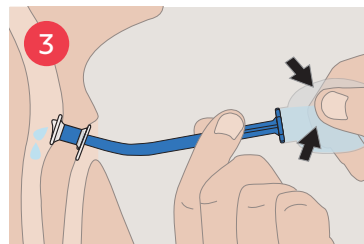


► **FLUSH** your voice prosthesis with water or air.

Tip: Refer to the CareTip Voice Prosthesis Daily Care Routines for instructions.

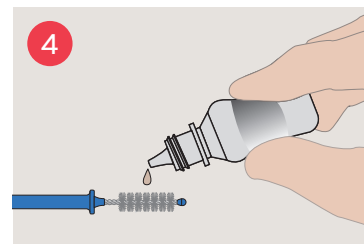

► **SWITCH** to the Brush labeled "Lubricant," and place a single drop of Provox ActiValve Lubricant on it only in the morning.

Avoid touching the Lubricant bottle to the Brush.

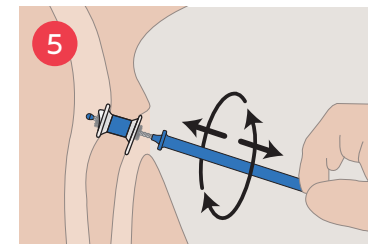

► **APPLY** the Lubricant by inserting the Brush into the center of the voice prosthesis. Carefully rotate the Brush while gently moving it back and forth.

Avoid touching the lubricated Brush to the skin inside your stoma.



6 Clean and disinfect both Brushes after use.

► **CLEAN** before inserting and after removal in warm, soapy water, then rinse.

Tip: Clean and disinfect both Brushes after use to ensure they are dry and ready for next time.

► **DISINFECT** by soaking using one of these methods:

- 70% Ethanol for 10 minutes **OR**
- 70% Isopropyl alcohol for 10 minutes **OR**
- 3% Hydrogen peroxide for 60 minutes.

Caution: Do not drip Lubricant into the lungs.



It is important to use just one drop to avoid excess Lubricant that could drip onto your skin or into your stoma or lungs.


Too much lubricant may also cause the valve to stick from build up.

Tips for successful use:

If you haven't talked for a while or when first waking up, you may find that the voice prosthesis valve is sticking and talking is more difficult. Cleaning and lubricating the voice prosthesis can help reduce sticking.

Only use Provox ActiValve Lubricant on the Provox Brush. Other lubricants or instruments may damage the Provox ActiValve.

Complete the Provox ActiValve User Card with a permanent marker and carry it with you at all times.

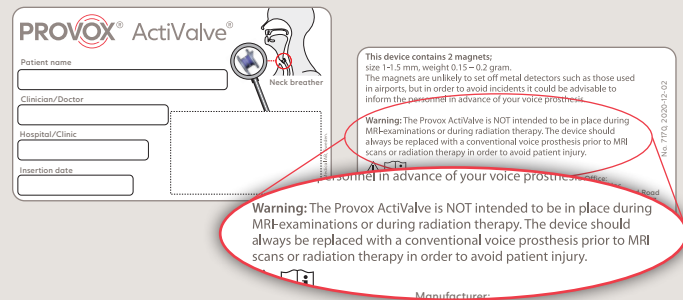

Take a picture of your User Card should you ever accidentally misplace it.

Tip for air travel

Although the magnets in the Provox ActiValve are unlikely to set off a metal detector (such as those used at airports), be sure to present your Provox ActiValve User Card before going through screening.

Medical procedure information



Always inform healthcare providers and emergency personnel about your Provox ActiValve voice prosthesis, and be sure to tell them that it contains magnets.

Show healthcare providers your Provox ActiValve User Card before undergoing any type of medical procedure or examination.

DO NOT UNDERGO



MRI EXAM



RADIATION THERAPY

**WITH THE PROVOX ACTIVEVALVE
VOICE PROSTHESIS IN PLACE.**

Watch the video "ActiValve Care and Maintenance":
[www.atosmedical.us/
videos/provox-activevalve-
care-and-maintenance](http://www.atosmedical.us/videos/provox-activevalve-care-and-maintenance)
or scan this QR code:



References:

- Mayo-Yáñez M, Chiesa-Estomba C, Lechien JR, Calvo-Henríquez C, Vaira LA, Cabo-Varela I. Long-term outcomes and cost-effectiveness of a magnet-based valve voice prosthesis for endoprosthesis leakage treatment. *Eur Arch Otorhinolaryngol*. 2022 Aug;279(8):4167-4172. doi: 10.1007/s00405-022-07313-x. Epub 2022 Feb 26. PMID: 35217904.
- Lewin JS, Baumgart LM, Barrow MP, Hutcheson KA. Device Life of the Tracheoesophageal Voice Prosthesis Revisited. *JAMA Otolaryngol Head Neck Surg*. 2017 Jan 1;143(1):65-71. doi: 10.1001/jamaoto.2016.2771. PMID: 27684464; PMCID: PMC5322740.
- Graville DJ, Palmer AD, Andersen PE, Cohen JI. Determining the efficacy and cost-effectiveness of the ActiValve: results of a long-term prospective trial. *Laryngoscope*. 2011 Apr;121(4):769-76. doi: 10.1002/lary.21380. Epub 2011 Mar 4. PMID: 21381042.
- Hilgers FJ, Ackerstaff AH, Balm AJ, Van den Brekel MW, Bing Tan I, Persson JO. A new problem-solving indwelling voice prosthesis, eliminating the need for frequent Candida- and "underpressure"-related replacements: Provox ActiValve. *Acta Otolaryngol*. 2003 Oct;123(8):972-9. doi: 10.1080/00016480310015371. PMID: 14606602.
- Soolsma J, van den Brekel MW, Ackerstaff AH, Balm AJ, Tan B, Hilgers FJ. Long-term results of Provox ActiValve, solving the problem of frequent candida- and "underpressure"-related voice prosthesis replacements. *Laryngoscope*. 2008 Feb;118(2):252-7. doi: 10.1097/MLG.0b013e318159ebde. PMID: 18090869.
- Kress P, Schäfer P, Schwerdtfeger FP, Rösler S. Are modern voice prostheses better? A lifetime comparison of 749 voice prostheses. *Eur Arch Otorhinolaryngol*. 2014 Jan;271(1):133-40. doi: 10.1007/s00405-013-2611-0. Epub 2013 Jun 29. PMID: 23812585; PMCID: PMC3889693.
- Petersen JF, Lansaat L, Timmermans AJ, van der Noort V, Hilgers FJM, van den Brekel MWM. Postlaryngectomy prosthetic voice rehabilitation outcomes in a consecutive cohort of 232 patients over a 13-year period. *Head Neck*. 2019 Mar;41(3):623-631. doi: 10.1002/hed.25364. Epub 2019 Jan 7. PMID: 30614644; PMCID: PMC6590326.